


EXPT B-26

AMES TEST

CIG SAMPLE NO 2AA-
SMOKE TYPE -
RUN NO -1
S9 DETAILS AR13
DATE 13/1/84
FILENAME B-262AA---1

DOSE UG.	COLONIES / PLATE			MEAN	CYTO. TOX.
	PLATE 1	PLATE 2	PLATE 3		
0	39.3	38	28	35.1	0
0.3	80.7	89	91.7	87.1	-
0.6	382.3	371	285	346.1	-
1.0	468.3	588.3	481	512.5	0

101014758

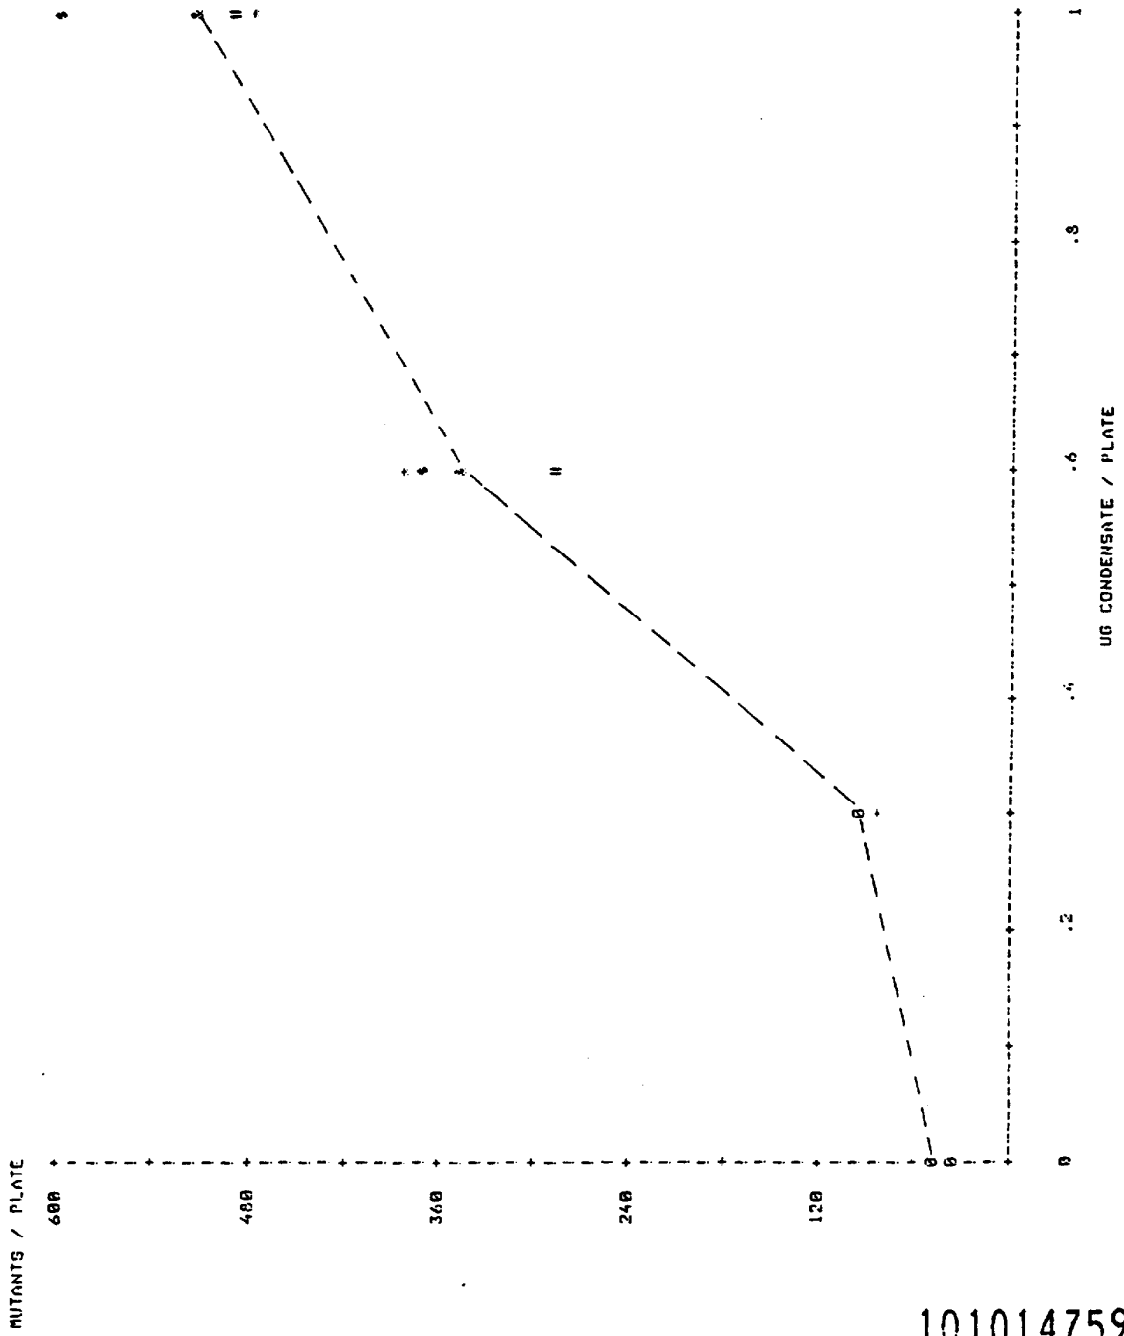

KEY: * -PLATE1 * -PLATE2 * -PLATE3 * -MEAN * FILENAME=0-26200---1

101014759