


EXPT 8-26

AMES TEST

CIG SAMPLE NO 2AA-
 SMOKE TYPE -
 RUN NO -2
 S9 DETAILS +AR13
 DATE 15/1/84
 FILENAME 8-262AA---2

DOSE UG.	COLONIES / PLATE			MEAN	CYTO. TOX.
	PLATE 1	PLATE 2	PLATE 3		
0	48.3	53	54.7	49.3	-
0.3	85.7	98.7	72	85.5	-
0.6	202.7	201.3	184.7	196.2	-
1.0	446	503	524.7	491.2	-

101014783

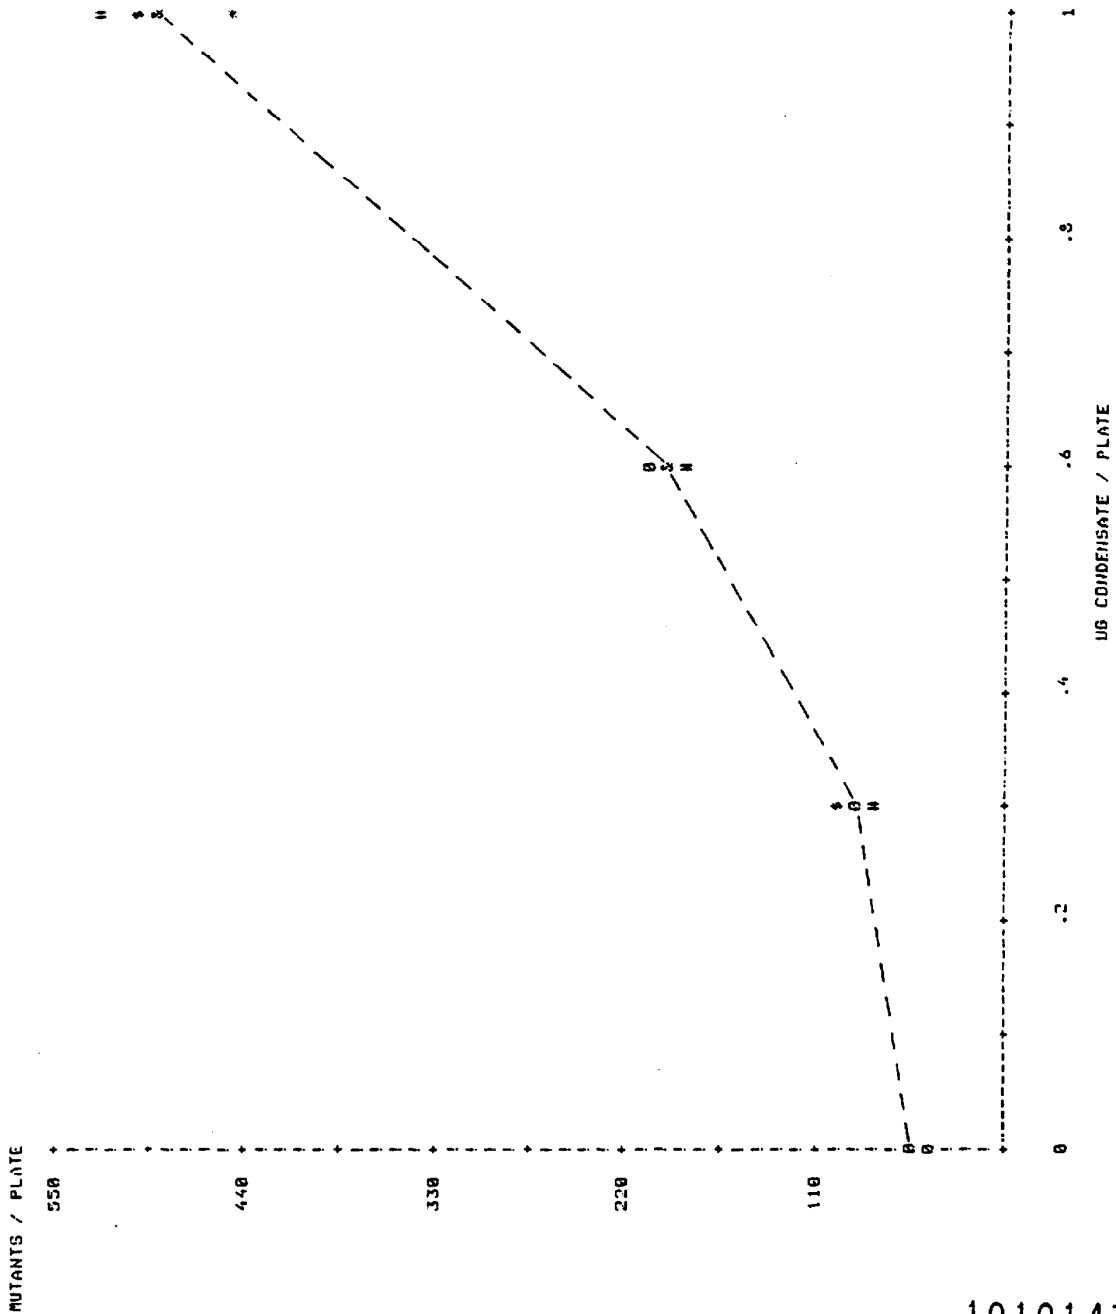

KEY: +-PLATE1 \$-PLATE2 H-PLATE3 S-NEAR FILENAME-6-263JA

101014784