


EXPT B-26

AMES TEST

CIG SAMPLE NO P161
SMOKE TYPE M
RUN NO -3
SP DETAILS +AR13
DATE 23/1/84
FILENAME B-26P161M-3

DOSE UG.	COLONIES / PLATE			MEAN	CYTO. TOX.
	PLATE 1	PLATE 2	PLATE 3		
0	39.7	36.3	36.3	37.4 51.2	0
50	76	58	67.3	67.1 102.7	-
100	95.7	118	81.7	98.5 150.7	-
150	106	103	138	115.7 177.0	-
200	132.7	146.7	130.3	136.6 209.0	-
250	169.3	196.7	176.7	180.9 276.8	-
300	208.3	218.3	215.3	214 327.4	0

101014804

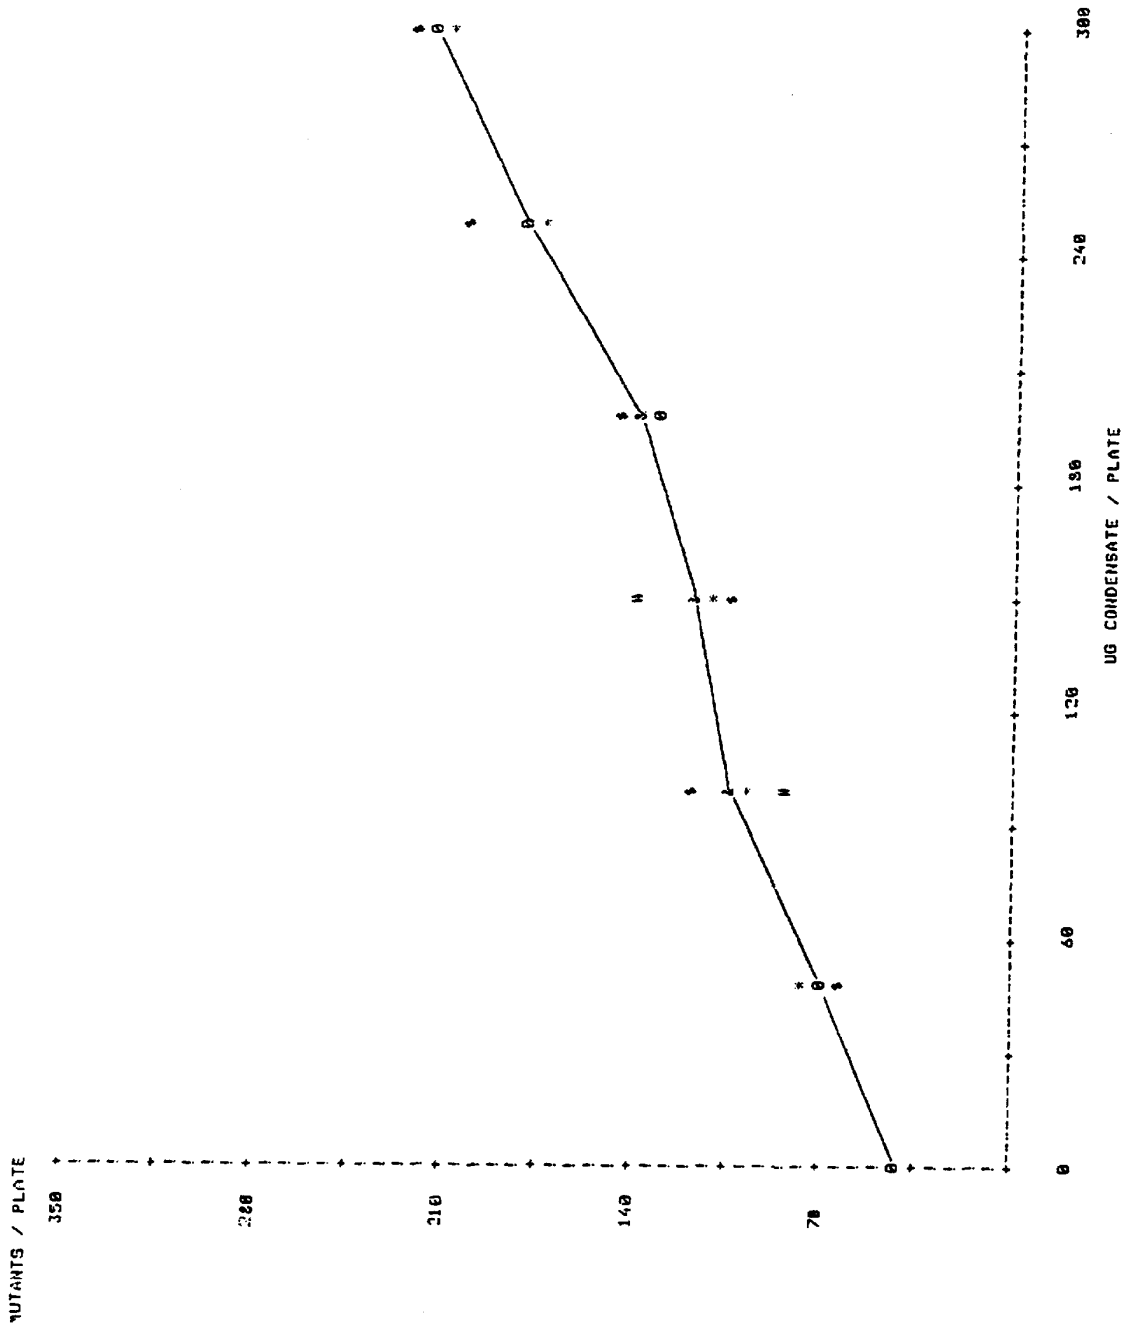

KEY: --PLATE1 \$-PLATE2 *-PLATE3 N-PLATE3 \$--MEAN FILENAME: 8-26P161M-3

10101400